

## Rat TGF-Beta 3 AccuSignal™ ELISA Kit - KOA0630

AccuSignal high sensitivity sandwich ELISA (Enzyme-Linked Immunosorbent Assay) Kit is *an in vitro* enzyme-linked immunosorbent assay designed for the quantitative detection of Rat TGF-Beta 3 in cell culture supernatants, serum, plasma (EDTA) and urine.

### I. KIT COMPONENTS

Rat TGF-Beta 3 AccuSignal™ ELISA Kit			
Component	Catalog Number	Description	Size
Antibody Coated ELISA Plate	KOA0630A	plate pre-coated with anti-Rat TGF-Beta 3 antibody	1
Target Protein Standard	KOA0630B	lyophilized recombinant Rat TGF-Beta 3	2 vials (10 ng/vial)
Biotinylated Detection Antibody	KOA0630C	biotinylated anti-rat TGF-BETA 3 antibody	130 µl (dilution 1:100)
ABC Complex	KAB0101	Avidin-Biotin-Peroxidase Complex (ABC)	130 µl (dilution 1:100)
Sample Diluent	KAE0101	sample diluent buffer	30 ml
Antibody Diluent	KAF0101	antibody diluent buffer	12 ml
ABC Diluent	KAG0101	ABC diluent buffer	12 ml
Substrate Solution	KAC0101	TMB color developing reagent	10 ml
Stop Solution	KAD0101	TMB stop solution	10 ml
Adhesive Cover	-	Adhesive cover	4

### II. STORAGE CONDITIONS

Store at 4°C for 6 months, or at -20°C for 12 months from date of manufacture. Avoid multiple freeze-thaw cycles.

### III. INTRODUCTION

Rat TGF-Beta 3 ELISA Kit is based on standard sandwich enzyme-linked immune-sorbent assay technology. This assay employs a monoclonal antibody specific for TGF-BETA 3 pre-coated onto 96-well plate. Standards (Expression system for standard: sf21; Immunogen sequence: A301-S412) and test samples are pipetted into the wells, and a biotinylated detection polyclonal antibody from goat specific for TGF-BETA 3 is added to the wells. The wells are washed with PBS or TBS buffer. After washing away unbound biotinylated antibody, Avidin-Biotin-Peroxidase Complex is added to the wells and unbound conjugates are washed away with PBS or TBS buffer. HRP substrate TMB solution is added to the wells to visualize HRP enzymatic reaction. TMB is catalyzed by HRP to produce a blue color product. The addition of stop solution changes the color from blue to yellow. The density of yellow is proportional to the amount of Rat TGF-Beta 3 amount captured in plate.

#### IV. REQUIRED EQUIPMENT AND REAGENTS

- Microplate reader in standard size
- Automated plate washer
- Adjustable pipettes and pipette tips
- Clean tubes and Eppendorf tubes
- Washing buffer (neutral PBS or TBS)
  - Preparation of 0.01M TBS:  
Add 1.2g Tris, 8.5g NaCl; 450µl of purified acetic acid or 700µl of concentrated hydrochloric acid to 1000 ml distilled water and adjust pH to 7.2-7.6. Finally, adjust the total volume to 1L.
  - Preparation of 0.01 M PBS:  
Add 8.5 g sodium chloride, 1.4 g Na<sub>2</sub>HPO<sub>4</sub> and 0.2 g NaH<sub>2</sub>PO<sub>4</sub> to 1000 ml distilled water and adjust pH to 7.2-7.6. Finally, adjust the total volume to 1L.

#### V. GENERAL CONSIDERATIONS

Please read the following instructions before starting the experiment.

- To inspect the validity of experimental operation and the appropriateness of sample dilution proportions, pilot experiment using standards and a small number of samples is recommended.
- The TMB Color Developing agent is colorless and transparent before using, contact us if it is not the case.
- Before using the Kit, briefly spin down the vials.
- For statistical reasons, we recommend both standard and samples should be assayed with a minimum of two replicates (duplicates).
- Do not let 96-well plate to dry, this will inactivate active components on plate.
- Avoid cross contamination of samples or reagents by changing tips between sample, standard and reagent additions.
- Do not mix or substitute reagents or materials from other kit lots or vendors.
- In order to avoid marginal effect of plate incubation due to temperature difference (reaction may be stronger in the marginal wells), it is suggested that the diluted ABC and TMB solution be pre-warmed in 37°C for 30 min before using.

#### VI. SANDWICH ELISA PROTOCOL

##### A. Sample Preparation

Store samples to be assayed within 24 hours at 2-8°C. For long-term storage, aliquot and freeze samples at -20°C. Avoid repeated freeze-thaw cycles.

- **Serum:**  
Allow the serum to clot in a serum separator tube (about 4 hours) at room temperature.  
Centrifuge at approximately 1000 X g for 15 min. Analyze the serum immediately or aliquot and store at -20°C.

- **Cell culture supernatants:**  
Remove particulates by centrifugation, assay immediately or aliquot and store at -20°C.
- **Plasma:**  
Collect plasma using heparin or EDTA as an anticoagulant. Centrifuge for 15 min at 1000 x g within 30 min of collection. Assay immediately or aliquot and store at -20°C.
  - \*Note: it is important not to use anticoagulants other than those listed above to treat plasma. Other anticoagulants could block the antibody binding site.
- **Urine:**  
Collect the first urine of the day, micturate directly into a sterile container. Remove impurities by centrifugation, assay immediately or aliquot and store samples at -20°C.

## B. Sample Activation

- Note: To detect TGFB3 in samples, you need to activate TGFB3 in samples prior to the assay.
- Solution A: 1N HCl: add 8.33ml of 12N HCl into 91.67ml of H<sub>2</sub>O.
- Solution B: 1.2N NaOH/0.5M HEPES: add 12ml of 10N NaOH and 11.9g HEPES into 75ml of H<sub>2</sub>O, add H<sub>2</sub>O to adjust volume to 100ml.
  - Cell culture supernates, urine: add activating reagent pro rata, i.e. add 20µl of Solution A into 100µl of sample, 10 min later, add 20µl of Solution B. PH 7.0-7.6.
  - Serum, plasma (EDTA): add activating reagent pro rata, i.e. add 20µl of Solution A into 40µl of sample, 10 min later, add 20µl of Solution B. PH 7.0-7.6.
  - It is unnecessary to activate the recombinant TGF-beta 3.
- Sample was diluted partly after adding activating reagent, so please pay attention to this when calculate target protein concentration.

## C. Sample Dilution

Please note that levels of the target protein may vary between different samples. Estimation of the concentration of a target protein in the sample and the optimal dilution factors for each sample must be determined by the investigator. The target protein concentration should be estimated, and appropriate sample dilutions should be selected such that the final protein concentration lies near the middle of the linear dynamic range of the assay. It is recommended to prepare 150 µl of sample for each replicate to be assayed. The samples should be diluted with sample diluent and mixed gently.

Following are the suggested guidelines for sample dilution. **The samples must be mixed well with the diluent buffer.**

- **High target protein concentration (20,000pg/ml-200,000pg/ml)**  
The working dilution should be 1:100. For example, add 1µl sample into a tube with 99µl sample diluent buffer.
- **Medium target protein concentration (2000pg/ml-20,000pg/ml)**  
The working dilution should be 1:10. For example, add 10µl sample into a tube with 90µl sample diluent buffer.
- **Low target protein concentration (31.2pg/ml-2000pg/ml)**  
The working dilution should be 1:2. For example, add 50µl sample into a tube with 50µl sample diluent buffer.
- **Very Low target protein concentration (0pg/ml-31.2pg/ml)**  
No dilution necessary, or the working dilution should be 1:2.

## D. Reagent Preparation

### Reconstitution of the Rat TGF-Beta 3 standard:

TGF-BETA 3 standard solution should be prepared no more than 2 hours prior to the experiment. Two vials of TGF-BETA 3 standard (10ng/vial) are provided with each kit. Use one vial/experiment.

- Reconstitute standard to a stock concentration of a 10ng/mL using 1mL of sample diluent. Keep the vial at room temperature for 10 min and mix thoroughly.
- Label tubes 1-8. 2000pg/ml (tube#1), 1000pg/ml (tube#2), 500pg/ml (tube#3), 250pg/ml (tube#4), 125pg/ml (tube#5), 62.5pg/ml (tube#6), 31.25pg/mL (tube#7), and 0.0 blank (tube#8) respectively.
- For preparation of standard #1, add 0.2ml of the above TGF-BETA 3 stock standard solution into 0.8ml of sample diluent buffer into tube#1 and mix thoroughly.
- For preparation of standard #2, transfer 300 $\mu$ l from tube #1 to tube #2 and mix thoroughly.
- Transfer 300 $\mu$ l from tube #2 to tube #3 and mix thoroughly and continue to prepare further serial dilutions.
- Tube 8 is left blank.

**Note:** The standard solutions are best used within 2 hours. The 10,000pg/ml standard solution should be stored at 4°C for up to 12 hours, or at -20°C for up to 48 hours. Avoid repeated freeze-thaw cycles.

### Preparation of biotinylated anti-Rat TGF-Beta 3 antibody working solution:

The solution should be prepared no more than 2 hours prior to the experiment.

- The total volume should be 0.1ml/well x (the number of wells). Prepare 100-200 $\mu$ l more of the solution than the total volume required to compensate for pipetting errors.
- Biotinylated anti-Rat TGF-Beta 3 antibody should be diluted 1:100 with the antibody diluent buffer and mixed thoroughly. For example, add 1 $\mu$ l Biotinylated Anti-Rat TGF-Beta 3 antibody to 99 $\mu$ l antibody diluent buffer.

### Preparation of Avidin-Biotin-Peroxidase Complex (ABC) working solution:

The solution should be prepared no more than 1 hour prior to the experiment.

- The total volume should be: 0.1 ml/well x (the number of wells). Prepare 0.1-0.2 ml more of the solution than total volume required.
- Avidin-Biotin-Peroxidase Complex (ABC) should be diluted 1:100 with the ABC dilution buffer and mixed thoroughly. For example, add 1 $\mu$ l ABC to 99 $\mu$ l ABC diluent buffer.

## E. Assay Procedure

ABC working solution and TMB substrate reagent should be warmed at 37°C for 30 min prior to use. Samples and reagents should be mixed thoroughly and evenly after dilution. A standard curve for TGF-

BETA 3 detection should be prepared for each experiment. It is recommended to determine sample fold dilution by simple estimation of TGF-BETA 3 amount in the samples.

1. Aliquot 100µl per well of each standard, sample, or control into wells. **It is recommended to assay all standards, controls and samples in duplicate.**
2. Seal the plate with provided adhesive plastic cover and incubate at RT for 120 min or 37°C for 90 min.
3. Remove the cover and discard the solution. Invert the plate and blot it against clean paper towels or other absorbent material. Do NOT let the wells dry completely at any time.
4. Add 100µl of biotinylated anti-Rat TGF-Beta 3 antibody working solution to each well, seal the plate with adhesive plastic cover and incubate at RT for 90 min or 37°C for 60 min.
5. Discard the solution and wash the plate 3 times with 0.01M TBS or 0.01M PBS (wash buffer) and each time let washing buffer stay in the wells for ~1 min. Wash by filling each well with 300µl of wash buffer using a multi-channel pipette or auto washer. Complete removal of liquid at each step is essential to good performance. (Note: for automated washing, aspirate all wells and wash THREE times with PBS or TBS buffer, overfilling the wells with PBS or TBS buffer). After the last wash, remove any remaining wash buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels or other absorbent material.
6. Add 100µl of prepared ABC working solution to each well, seal the plate and incubate at RT for 40min or 37°C for 30 min.
7. Wash plate 5 times with 0.01M TBS or 0.01M PBS as described in step 5.
8. Add 90µl of TMB substrate reagent to each well, seal the plate and incubate at RT for 30 min or at 37°C for 15-25 min in the dark. (Note: the optimal incubation time should be determined by the end user).
9. Add 100µl of stop solution to each well. The color will change to yellow immediately.
10. Read at 450 nm in a microplate reader within 30 min after adding the stop solution.

## Calculations

For calculations, (the relative O.D.450) = (the O.D.450 of each well) – (the O.D.450 of Zero well). The standard curve can be plotted as the relative O.D.450 of each standard solution (Y) vs. the respective concentration of the standard solution (X). The Rat TGF-Beta 3 concentration of the samples can be interpolated from the standard curve.


**Note:** if the samples measured were diluted, multiply the concentrations obtained from interpolation by the dilution factor.

## VII. DATA OBTAINED FROM RAT TGF-BETA 3

Concentration (pg/ml)	0	31.2	62.5	125	250	500	1000	2000
O.D	0.042	0.125	0.214	0.345	0.581	1.119	1.612	2.125

(TMB reaction incubation at 37°C for 25-30min)

### VIII. RAT TGF-BETA 3 ACCUSIGNAL™ ELISA KIT STANDARD CURVE

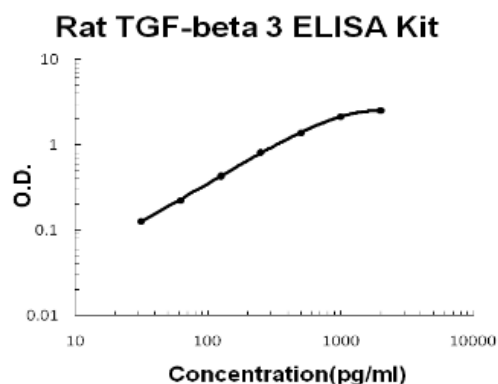

This standard curve was generated for demonstration purpose only (A standard curve must be run with each assay).

<b>Range</b>	31.2pg/ml-2000pg/ml
<b>Sensitivity</b>	<10pg/ml
<b>Specificity</b>	Natural and recombinant Rat TGF-Beta 3
<b>Cross-reactivity</b>	There is no detectable cross-reactivity with other relevant proteins.

### IX. INTRA AND INTER ASSAY PRECISION

**Intra-Assay Precision** (Precision within an assay): Three samples of known concentration were tested on one plate to assess intra-assay precision.

**Inter-Assay Precision** (Precision between assays): Three samples of known concentration were tested in separate assays to assess inter-assay precision.

	Intra-Assay Precision			Inter-Assay Precision		
Sample	1	2	3	1	2	3
<b>N</b>	16	16	16	24	24	24
<b>Mean(pg/ml)</b>	77	234	841	81	242	805
<b>Standard deviation</b>	5.22	14.97	42.89	7.12	18.15	41.86
<b>CV (%)</b>	7.7	6.4	5.2	8.8	7.5	5.2

## X. ASSAY SUMMARY

- Prepare all reagents, samples and standards as instructed.
- Add standards or samples to each well used. Incubate the plate at 37°C for 90 min. Do not wash.
- Add prepared biotinylated antibody to each well. Incubate the plate at 37°C for 60 min. Wash plate 3 times with 0.01M TBS or PBS.
- Add prepared ABC working solution. Incubate the plate at 37°C for 30 min. Wash plate 5 times with 0.01M TBS or TBS.
- Add TMB developing reagent to each well. Incubate the plate at 37°C in dark for 25-30 min.
- Add TMB stop solution. Read at 450nm.

## XI. TROUBLESHOOTING

### Weak or No Signal

Possible Cause	Solution
<b>Problem with the standard</b>	Use new sample Check that the standard is appropriately handled
<b>Incubation time too short</b>	Follow the exact guidelines for incubation time (If the problem persists, try incubating samples at 4°C overnight)
<b>Incubation temperature too low</b>	Ensure incubations are done at correct temperature Before proceeding
<b>Incompatible sample type</b>	Use sample that the assay is known to detect as a positive control (Include such control in your experiment)
<b>Incompatible assay buffer</b>	Ensure assay buffer is compatible with the target of interest
<b>Target present below detection limit</b>	Decrease dilution factor or concentrate samples
<b>Incorrect/Insufficient/No substrate</b>	Check the substrate identity Increase concentration or amount of substrate
<b>Antibody stored at 4°C for several weeks or subjected to repeat freeze-thaw cycles</b>	Use fresh aliquot of antibody that has been stored at -20°C or below
<b>Incorrect reagents added/prepared; Missing reagents</b>	Check protocol, ensure correct reagents are added in proper order and prepared to correct concentrations
<b>Expired/Contaminated reagents</b>	Prepare fresh/uncontaminated reagents

<b>Enzyme inhibitor present</b>	Avoid sodium azide in HRP reactions
<b>Incorrect storage of components</b>	Check storage conditions for the kit (Kit need to be stored at 4°C)
<b>Excessive plate washing</b>	Gently pipette wash buffer (manual method) Ensure correct pressure (automatic wash system)
<b>Wells dry out</b>	Cover plate using adhesive cover at all incubation times
<b>Plate read at incorrect detection wavelength</b>	Use recommended wavelength/filter Ensure plate reader is set correctly for substrate used
<b>Slow color development</b>	Prepare substrate immediately before use Allow longer incubation time Ensure stock solution is unexpired and uncontaminated

### Saturated Signal

Possible Cause	Solution
<b>High sample concentration</b>	Use higher sample dilutions (Determine the optimal dilutions by titration assay)
<b>Excessive substrate</b>	Decrease concentration or amount of substrate: The substrate provided with the ELISA kit might require further dilution
<b>Substrate color changed before use</b>	Prepare substrate immediately before use
<b>Non-specific antibody binding</b>	Use affinity-purified antibody and preferably one that is pre-adsorbed.
<b>Incubation time too long</b>	Follow the exact guidelines (If the problem persists, try incubating samples at 4°C overnight)
<b>Excessive antibody</b>	Repeat the assay with lower antibody concentrations to find the optimal one for your experiment
<b>Contaminated buffers or HRP</b>	Prepare and use fresh buffers
<b>Insufficient washing</b>	Follow the exact guidelines At the end of each washing step, flick the plate over a sink and dry the plate on a paper towel
<b>Plate adhesive cover not used or re-used</b>	During incubations, cover plates with adhesive cover. Use a fresh cover every time the used cover is removed from the plate
<b>Plate read at incorrect wavelength</b>	Use recommended wavelength/filter Ensure plate reader is set correctly for the substrate used
<b>Excess time before plate reading</b>	Read your plate within 30 minutes after adding the substrate (If the reading is not performed within this time frame, add a stopping solution after sufficient color is developed in the plate)

### High Background

Possible Cause	Solution
<b>Insufficient washing</b>	Follow the exact guidelines At the end of each washing step, flick the plate over a sink and pat dry the plate on a paper towel
<b>Excessive antibody</b>	Repeat the assay with lower antibody concentrations to find the optimal one for your experiment



<b>Excessive substrate</b>	Decrease concentration or amount of substrate
<b>Cross reactivity</b>	Run appropriate controls
<b>Non-specific antibody binding</b>	Use affinity-purified antibody and preferably one that is pre-adsorbed
<b>Insufficient Tween in buffers</b>	Use PBS or TBS containing 0.05% Tween
<b>Suboptimal salt concentration in washing buffer</b>	Optimize salt concentration as high concentration can reduce non-specific interactions
<b>Incubation temperature too high</b>	Optimize incubation temperature for your assay (antibodies bind optimally at very specific temperature)
<b>Reagents were not mixed properly</b>	Thoroughly mix all reagents and samples before pipetting solutions into wells
<b>Blanks contaminated with samples</b>	Change pipette tips when switching between blanks and samples
<b>Sample contaminated with enzymes</b>	Test samples with substrate alone to check for contaminating enzymes
<b>Contaminated TMB substrate</b>	Use a clean container to check that the substrate is not contaminated (TMB substrate should be clear and colorless before adding to wells)
<b>Substrate exposed to light</b>	Carry out substrate incubation in dark
<b>Evaporation of solution from well during incubation</b>	Always incubate with a cover on the plate
<b>Incubation time too long</b>	Follow the exact guidelines for incubation times (If the problem persists, try incubating samples at 4°C overnight)
<b>Incorrect standard curve dilutions</b>	Check pipetting techniques Check calculations
<b>Unstopped color development</b>	Use Stopping solution to prevent over-development
<b>Excessive time lapsed before plate reading</b>	Read your plate within 30 minutes after adding the substrate (If the reading is not performed within this time frame, add a stopping solution after sufficient color is developed in the plate)
<b>Incorrect plate reading setting</b>	Use recommended wavelength/filter Ensure plate reader is set correctly for the substrate used

### Low Sensitivity

Possible Cause	Solution
<b>Improper storage of ELISA kit</b>	Store all reagents as recommended
<b>Insufficient target</b>	Reduce sample dilution or concentrate sample
<b>Inactive substrate</b>	Ensure reporter enzyme has the expected activity
<b>Insufficient substrate</b>	Increase concentration or amount of substrate
<b>Incompatible sample type</b>	Include positive control in your experiment
<b>Interfering ingredients in buffers and sample</b>	Check reagents for any interfering chemicals, e.g. sodium azide in antibodies inhibit HRP enzyme; EDTA used as anti-coagulant for plasma collection inhibits enzymatic reactions
<b>Mixing or substituting reagents from different kits</b>	Avoid mixing components from different kits
<b>Incorrect plate reading setting</b>	Use recommended wavelength/filter Ensure plate reader is set correctly for the substrate used

### Poor Standard Curve Generation

Possible Cause	Solution
<b>Improper standard solution</b>	Confirm dilutions are done correctly Prepare new standard curve as appropriate
<b>Standard improperly reconstituted</b>	Briefly spin vial before opening Inspect for undissolved material after reconstituting
<b>Standard degraded</b>	Store and handle standard as recommended Prepare standards no more than two hours before use
<b>Pipetting error</b>	Use calibrated pipettes and proper pipetting technique
<b>Insufficient washing</b>	Follow the exact guidelines At the end of each washing step, flick the plate over a sink and pat dry the plate on a paper towel
<b>Poorly mixed reagents</b>	Thoroughly mix reagents
<b>Plates stacked during incubation</b>	Keep plates separated if not using rotating plates

### Poor Replicate Data

Possible Cause	Solution
<b>Bubbles in wells</b>	Ensure no bubbles are present prior to reading the plate
<b>Insufficient washing of wells</b>	Carefully wash wells Check that all ports of the plate washer are unobstructed
<b>Incomplete reagent mixing</b>	Ensure all reagents are mixed thoroughly
<b>Inconsistent pipetting</b>	Use calibrated pipettes and proper pipetting techniques Use a new cover every time the used cover is removed from the plate
<b>Inconsistent sample preparation or storage</b>	Ensure consistent sample preparation and optimal sample storage (e.g. minimize freeze/thaw cycles)
<b>Particulates in samples</b>	Remove the particulates by centrifugation
<b>Cross-well contamination</b>	Ensure plate covers and pipette tips are not contaminated with reagents
<b>Edge effect (higher or lower OD in peripheral wells than in central wells)</b>	Ensure plates and reagents are kept at temperatures as instructed During incubation, seal the plate completely and avoid stacking plates

### Inconsistent Assay-to-Assay Results

Possible Cause	Solution
<b>Insufficient washing of wells</b>	Carefully wash wells Check that all ports of the plate washer are unobstructed
<b>Varied incubation temperatures</b>	Adhere to recommended incubation temperature
<b>Variation in protocol</b>	Adhere to the same protocol from experiment to experiment
<b>Plate cover not used or re-used</b>	During incubations, cover plates with plate cover Use a new cover every time the used one is removed
<b>Incorrect dilutions</b>	Confirm dilutions are done correctly for standard solutions Prepare new standard curve as appropriate
<b>Contaminated buffers</b>	Prepare and use fresh buffers

## Slow Color Development

Possible Cause	Solution
<b>Substrates too old, contaminated or used at incorrect pH</b>	Prepare fresh substrates at correct pH
<b>Expired/Contaminated solutions</b>	Prepare fresh reagents before use
<b>Incorrect incubation temperature</b>	Ensure plates and reagents are kept at temperatures as instructed During incubation, seal the plate completely and avoid stacking plates
<b>Low antibody concentration</b>	Repeat the assay with higher antibody concentrations to find the optimal one for your experiment

## Plate Imaging Problem

Possible Cause	Solution
<b>Oversaturated image after acquisition</b>	Use full resolution image to analyze results (Do not use jpeg or other compressed formats)
<b>Blurry spots in images</b>	Re-focus your camera before taking a new image
<b>Repeated pixel values or rectangular spots</b>	Use lower bin size, higher image resolution and/or lossless file type
<b>Flat standard in images</b>	Reduce acquisition time

## XII. RELATED PRODUCTS

Component	Catalog #	Size
10x TBS pH 7.5	<a href="#">MB-012</a>	1000 ml
10x TTBS pH 7.5	<a href="#">MB-013</a>	1000 ml
10X PBS pH 7.2	<a href="#">MB-008</a>	1000 ml
10x PBST pH 7.2	<a href="#">MB-075-1000</a>	1000 ml